

AD-A116 022


WATERVLIET ARSENAL NY
LASER INTERFEROMETER CALIBRATION STATION.(U)
OCT 81 R W CAMPOLMI, S J KRUPSKI
WVT-9A-8101

F/6 20/5


UNCLASSIFIED

NL

1 of 1
AC 5
- 20 -

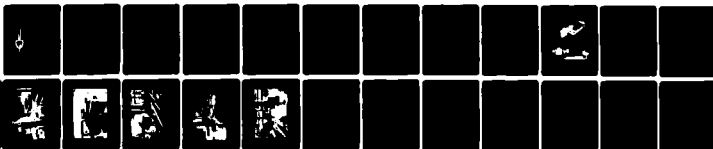

END
DATE
FILMED
7-82
DTIC

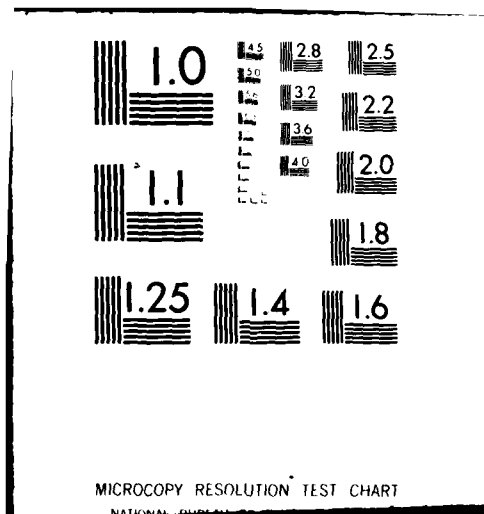

3



WVT-QA-8101

**LASER INTERFEROMETER
CALIBRATION STATION**

**R.W. CAMPOLMI
S.J. KRUPSKI**

OCTOBER 1981

AD A116022



**PRODUCT ASSURANCE DIRECTORATE
WATERVLIET ARSENAL
WATERVLIET, N.Y. 12189**

TECHNICAL REPORT

AMCMS No. 5397.OM.6350

Pron No. AW-8-P5191

**DTIC
ELECTE
JUN 24 1982
A**

APPROVED FOR PUBLIC RELEASE: DISTRIBUTION UNLIMITED

DTIC FILE COPY

82 36 039

DISCLAIMER

The findings in this report are not to be construed as an official Department of the Army position unless so designated by other authorized documents.

The use of trade name(s) and/or manufacture(s) does not constitute an official indorsement or approval.

DISPOSITION

Destroy this report when it is no longer needed. Do not return it to the originator.

SECURITY CLASSIFICATION OF THIS PAGE (When Data Entered)

REPORT DOCUMENTATION PAGE		READ INSTRUCTIONS BEFORE COMPLETING FORM
1. REPORT NUMBER WVT-QA-8101	2. GOVT ACCESSION NO. AU-A116-C22	3. RECIPIENT'S CATALOG NUMBER
4. TITLE (and Subtitle) Laser Interferometer Calibration Station		5. TYPE OF REPORT & PERIOD COVERED Final March 1978 to Sept 81
		6. PERFORMING ORG. REPORT NUMBER
7. AUTHOR(s) R. W. Campolmi and S. J. Krupski		8. CONTRACT OR GRANT NUMBER(s) AMCS No 5397. OM. 6350
9. PERFORMING ORGANIZATION NAME AND ADDRESS Product Assurance Directorate SARWV-QAE Watervliet Arsenal, Watervliet, NY 12189		10. PROGRAM ELEMENT, PROJECT, TASK AREA & WORK UNIT NUMBERS AW-8-P5191(-01-) M7-M7
11. CONTROLLING OFFICE NAME AND ADDRESS US Army Armament Command DRSAR-QAE Rock Island, IL 61299		12. REPORT DATE October 1981
		13. NUMBER OF PAGES 13
14. MONITORING AGENCY NAME & ADDRESS (if different from Controlling Office) Army Materials and Mechanics Research Ctr. AMXMR-MQ Watertown, MA 02172		15. SECURITY CLASS. (of this report) Unclassified
		15a. DECLASSIFICATION/DOWNGRADING SCHEDULE
16. DISTRIBUTION STATEMENT (of this Report) Approved for public release: distribution unlimited		
17. DISTRIBUTION STATEMENT (of the abstract entered in Block 20, if different from Report)		
18. SUPPLEMENTARY NOTES		
19. KEY WORDS (Continue on reverse side if necessary and identify by block number) Laser Interferometer Calibration Rifling Bar		
20. ABSTRACT (Continue on reverse side if necessary and identify by block number) The laser interferometer is a versatile tool, used for calibration over both long and short distances. It is considered traceable to the National Bureau of Standards. The system developed under this project was to be capable of providing for the calibration of many types of small linear measurement devices. The logistics of the original concept of one location for calibration of all mics, calipers, etc. at a large manufacturing facility proved unworkable. The equipment was instead used for the calibration of the large machines used to manufacture Cannon tubes.		

MATERIALS TESTING TECHNOLOGY PROGRAM (AMS 4931)

Report No. WVT-QA-8101

Title: Laser Interferometer
Calibration Station

THIS PROJECT HAS BEEN ACCOMPLISHED
AS PART OF THE US ARMY MATERIALS TESTING
TECHNOLOGY PROGRAM, WHICH HAS FOR ITS
OBJECTIVE THE TIMELY ESTABLISHMENT OF
TESTING TECHNIQUES, PROCEDURES OR
PROTOTYPE EQUIPMENT (IN MECHANICAL,
CHEMICAL, OR NONDESTRUCTIVE TESTING)
FOR MATERIEL/MATERIAL PROCURED OR
MAINTAINED BY AMC.



A

LIST OF ILLUSTRATIONS

1. Laser Interferometer Calibration Station - System Concept
2. Electronic Cartridge Calibration Station
3. Vertical and Horizontal Measurement Stations
4. Calibration of an Optical Comparator
5. Calibration Cart
6. Calibration Cart Setup for Rifling Bar Calibration
7. Laser Head, Remote Interferometer and Retroreflector
8. Rifling Bar with attached Rotary Encoder
9. Inspection Report
10. Plot of Rifling Bar Deviations

TABLE

1. System Parts List

ACKNOWLEDGEMENT

The authors wish to acknowledge Mr. Benjamin R. Taylor for the project concept and initial project development and Mr. Albert G. Gallo for subsequent project development.

1. INTRODUCTION

Previous investigations into the use of Laser Interferometry for linear distance measurements at Watervliet Arsenal^{1&2} resulted in the development of a Constant Force Device³ (CFD) and an improved method for calibrating both short and long length standards. A decision was made to build a general purpose system which could be used for calibration of micrometers, gage blocks, length standards, mechanical and electronic probes, cartridges, indicators, etc. This is a report on that project.

2. PRINCIPLES OF INTERFEROMETRY

A basic Laser Interferometer consists of a Laser Head which emits a double frequency, coherent beam of light; a combination beam splitter/retroreflector or remote interferometer; a moveable retroreflector also known as a "cube corner" and a Laser Display which contains a high speed electronic counter and a digital read-out. The electronics in the Display count the phase shifts generated by the laser beam being divided and recombined in the remote interferometer. One leg of the beam travels to the cube corner and the other leg provides a reference. The advantage of this system is that only the movement of the cube corner is measured.

¹ F.J. Audino and B.R. Taylor, "Applications of Laser Interferometry in Precision Measurements", Watervliet Arsenal Technical Report: WVT-QA-7405.

² "Functional Descriptions and Applications of Laser Inspection Systems", Product Assurance Pamphlet, AMSAR-WV-P-702-16, Sep 1975.

³ US Patent #3975100

The cube corner is attached to the object whose travel is being measured. The wavelength of this laser in a vacuum is a constant 6328 Angstroms or approximately .000024 inches. With compensation for air temperature, pressure and humidity, this constant is used to calculate the distance moved with a resolution of one millionth of an inch. This system also benefits from the fact that it is considered "a priori" traceable to the National Bureau of Standards and does not require routine calibration.⁴

3. SYSTEM CONCEPT

The Laser Interferometer Calibration Station Material Testing Technology Project was conceived as a method for quickly and accurately calibrating micrometers, length standards, electronic measurement cartridges (LVDTs), etc. Features of this system are: improved repeatability using the Constant Force Device; versatility; print on command, eliminating the need for the operator to interpret and record readings and the ability to handle an infinite number of calibration points with no degradation in accuracy.

The original system concept, shown in Fig. 1, had the laser mounted under the granite base with two right angle beam benders to bring the beam to the top surface of the table. The first station encountered by the beam was a micrometer measurement station. Two Constant Force Devices and a retroreflector were utilized to obtain readings at any location along the micrometers travel. The last station is the LVDT calibration station which is shown in Fig. 2. Fig. 3 depicts a later version of the station with a surface mounted laser. Air slides are incorporated to reduce friction and increase accuracy. This system has enough flexibility to allow additional stations to be added as the need arises.

⁴U.S. Dept of Commerce, N.B.S., Letter, dtd Oct 18, 1975

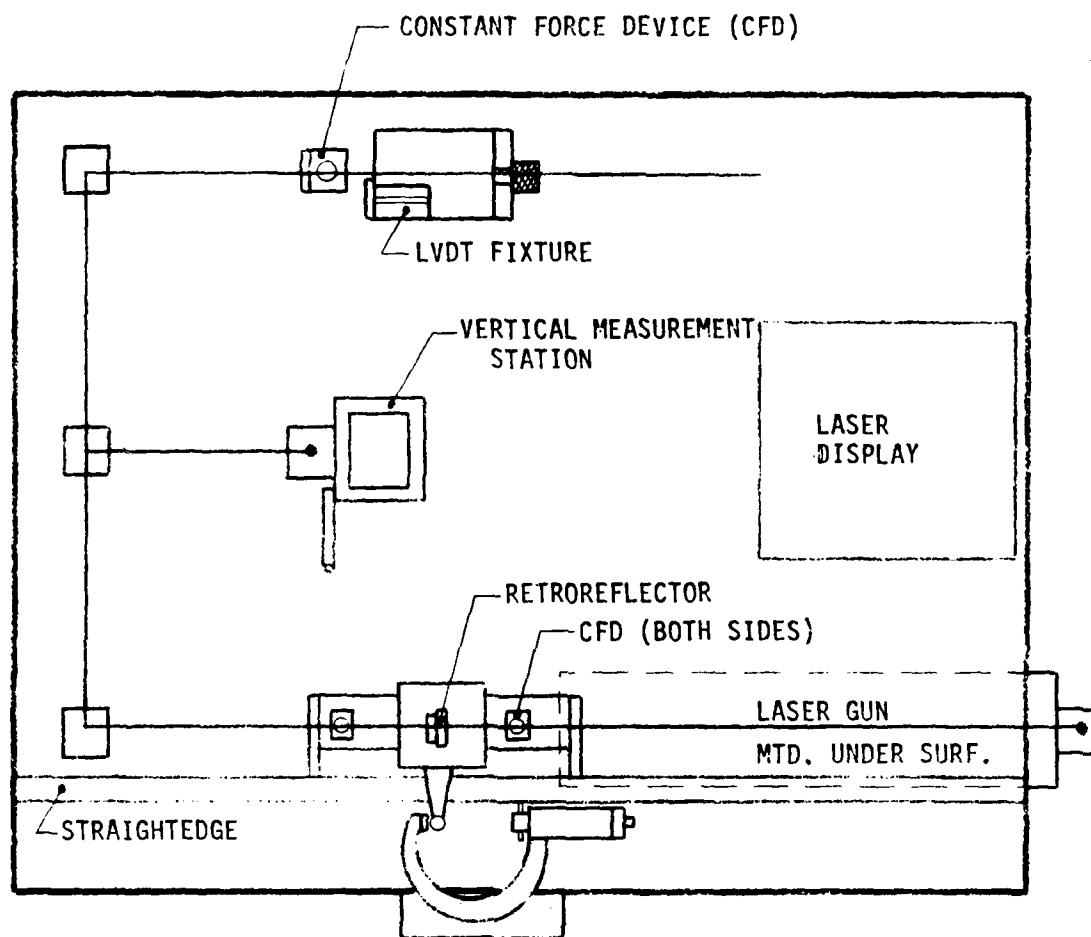


FIGURE 1. LASER INTERFEROMETER
CALIBRATION STATION-
SYSTEM CONCEPT

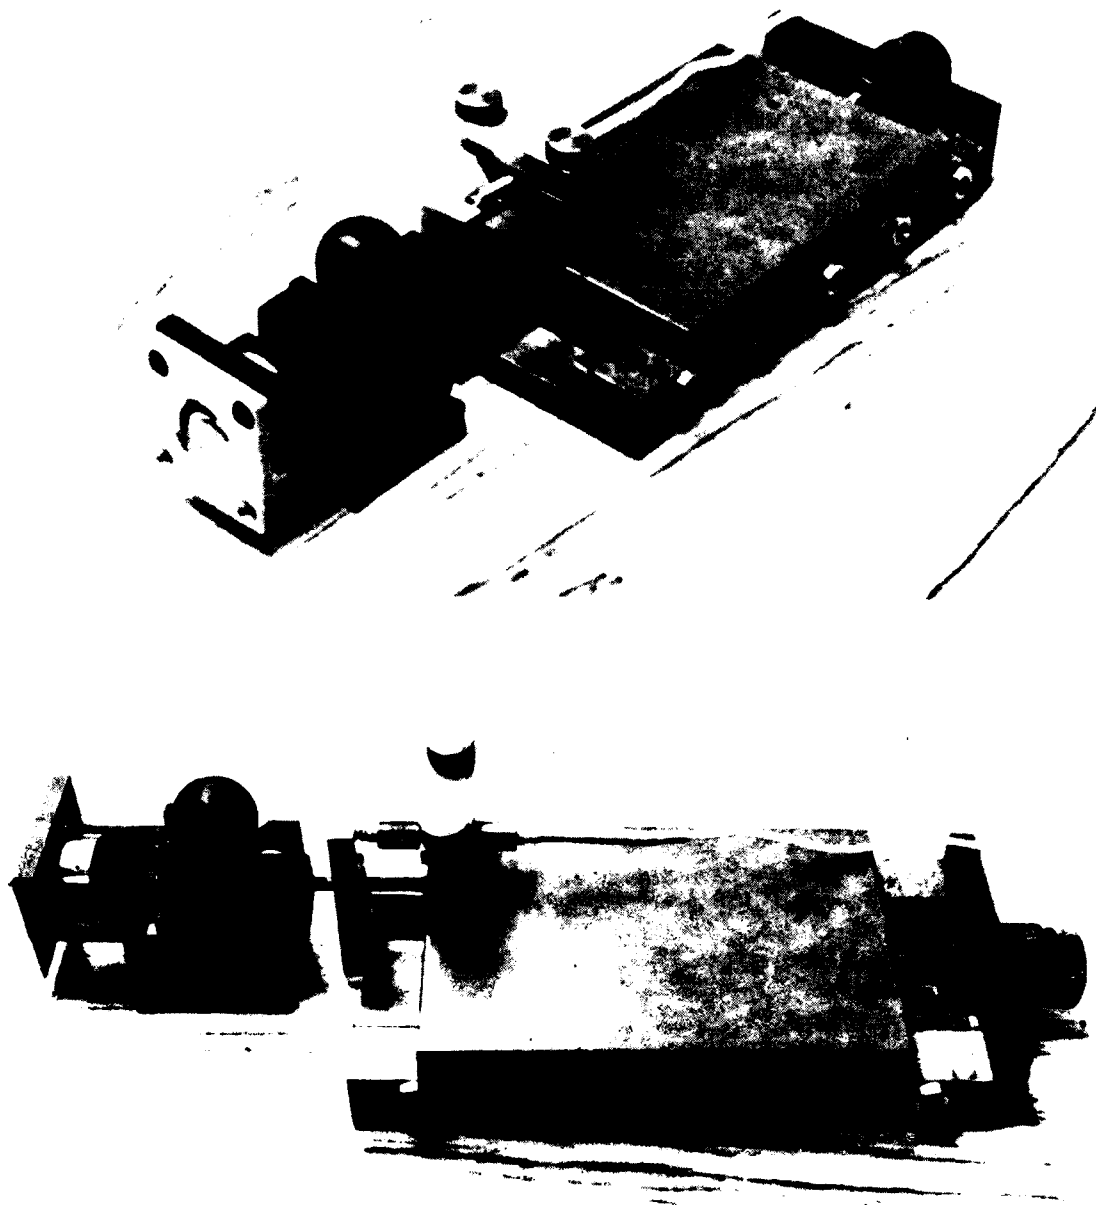


FIGURE 2. ELECTRONIC CARTRIDGE
CALIBRATION STATION

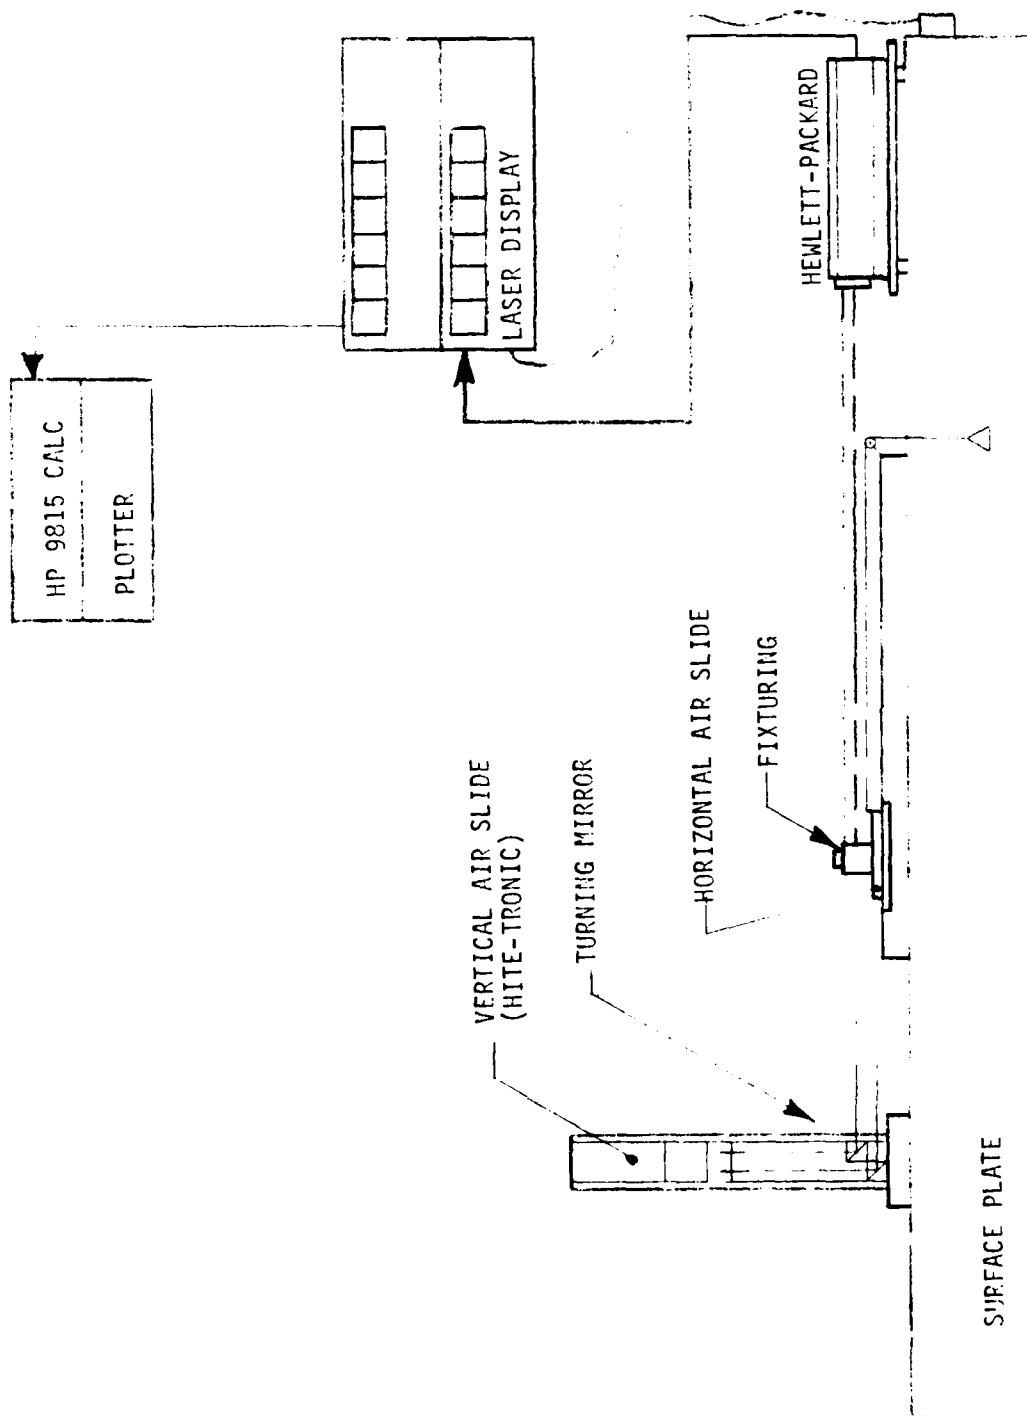


FIGURE 3. VERTICAL AND
HORIZONTAL MEASUREMENT
STATIONS

4. ACCOMPLISHMENTS

A Hewlett Packard Laser System (see Table 1) was purchased. This system was used in preliminary studies and during the design phase. The LVDT calibration station was built and tested. The fixture for the micrometer station went through several design iterations to produce a micrometer holding fixture which could accept mics from 1" to 12" for calibration, providing readings over the full range of travel, while retaining the required rigidity and convenience of operation. This last requirement was never totally fulfilled.

At this time, a logistical problem arose. Currently calibration of micrometers is done at the Surveillance Cribs located in each shop. If calibration was done at only one calibration station, it would be in the Product Assurance Gage Lab. Since the Lab is located away from the shop areas, mics brought to the Gage Lab for calibration would be out of service for a period of time and an additional cost incurred for transportation. Because there are insufficient mics to create a pool of "floaters", and because none of the organizations would bear the cost of transportation, the system soon acquired a "nice to have but not practical" status. As a result, it was decided that further expenditure of effort was not warranted.

5. ALTERNATE USES

Since the laser was purchased, it has been used to perform a variety of calibration functions. The passive Remote Interferometer and the retroreflector⁵ make the system ideal for calibration of N.C. machine tools, coordinate measuring machines (CMMs), rifling bars, etc. where calibration over long distances is involved.⁶

⁵R.R. Baldwin, G.B. Gordon, and A.F. Rude, "Remote Laser Interferometry", Hewlett Package Laser Measurement System Application Note 156-1.

⁶I.H. Hoffer, "Calibration of a Machine Tool", Hewlett Package Measurement System Application Note 156-4.

TABLE 1

System, Laser, HP 5526A
Laser Head
Laser Display

Interferometer, Remote HP 10565B & 10556A (Retro Reflector)

Bender, Beam HP 10558A

Retroreflector/Mount HP 10550B

Mirror, Turning HP 10557A

Case, Storage HP 10634A

Case, Storage HP 10635A

Mount, Reflector HP 10659A

Adapter, Straightness HP 10579A (2 pc)

Interferometer, Short-Range Straightness HP 10690A (Includes reflector)

Kit, Footspacing HP 10583A

Adapter, Straightness, Vertical HP 10693A

Splitter, Beam HP 10567A

Connecting Cables

System Laser HP 55262 Calculator Mod 9815A

System Parts List

Fig 4. shows the system being used to calibrate an optical comparator. Fig. 5 depicts the system installed on the Gage Surveillance Section's Calibration Cart. This Cart travels throughout the Arsenal shops where it is used for specialized calibration tasks. The laser has been especially valuable for the calibration of rifling bars.

With the exception of the 120mm tank gun which has a smooth bore, all large caliber gun tubes produced for the Army are rifled. Rifling consists of a number of equally spaced helical grooves cut in the bore of the gun. These grooves impart rotation to the projectile as it is launched, and the resulting spin provides in-flight stability. Manufacture of these grooves is done by a series of broaches, each slightly larger than the previous one, which are mounted on the end of a long bar called a rifling bar and pushed down the bore of the gun tube. A helical groove cut in the bar engages a pin in the machine which generates the required degree of rotation in the broaches and the resulting twist in the rifling.

Deviations in the rifling twist can cause variations in projectile performance, therefore, the twist of the rifling bars is periodically checked to insure conformance with the specification. The twist is expressed as _____ turns in _____ caliber, e.g. the 105mm M68 is one turn in eighteen calibers. A caliber is the bore size of the gun or 105mm. Therefore this may be stated as one turn in 1890mm or 74.412 inches.

Calibration of a rifling bar is shown in Figs. 6, 7 and 8. The bar itself is visible in all three photos. The helical groove can be seen in the extreme right hand side of Fig. 6 near the steady rest.



Figure 1. Illustration of an
EPIC 214 computer.

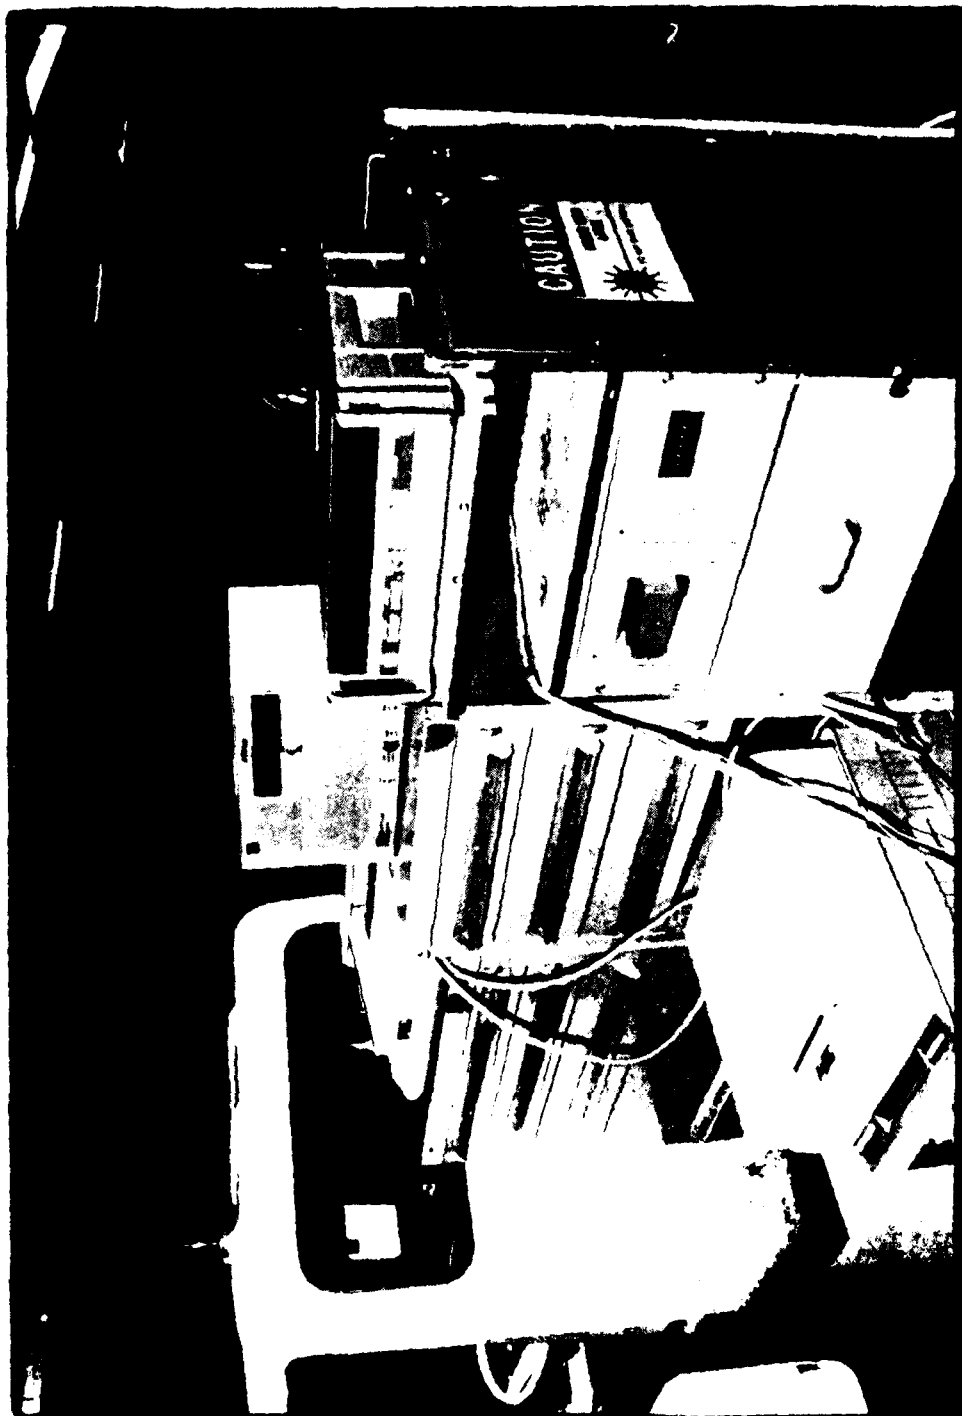


FIGURE 5. CALIBRATION CART

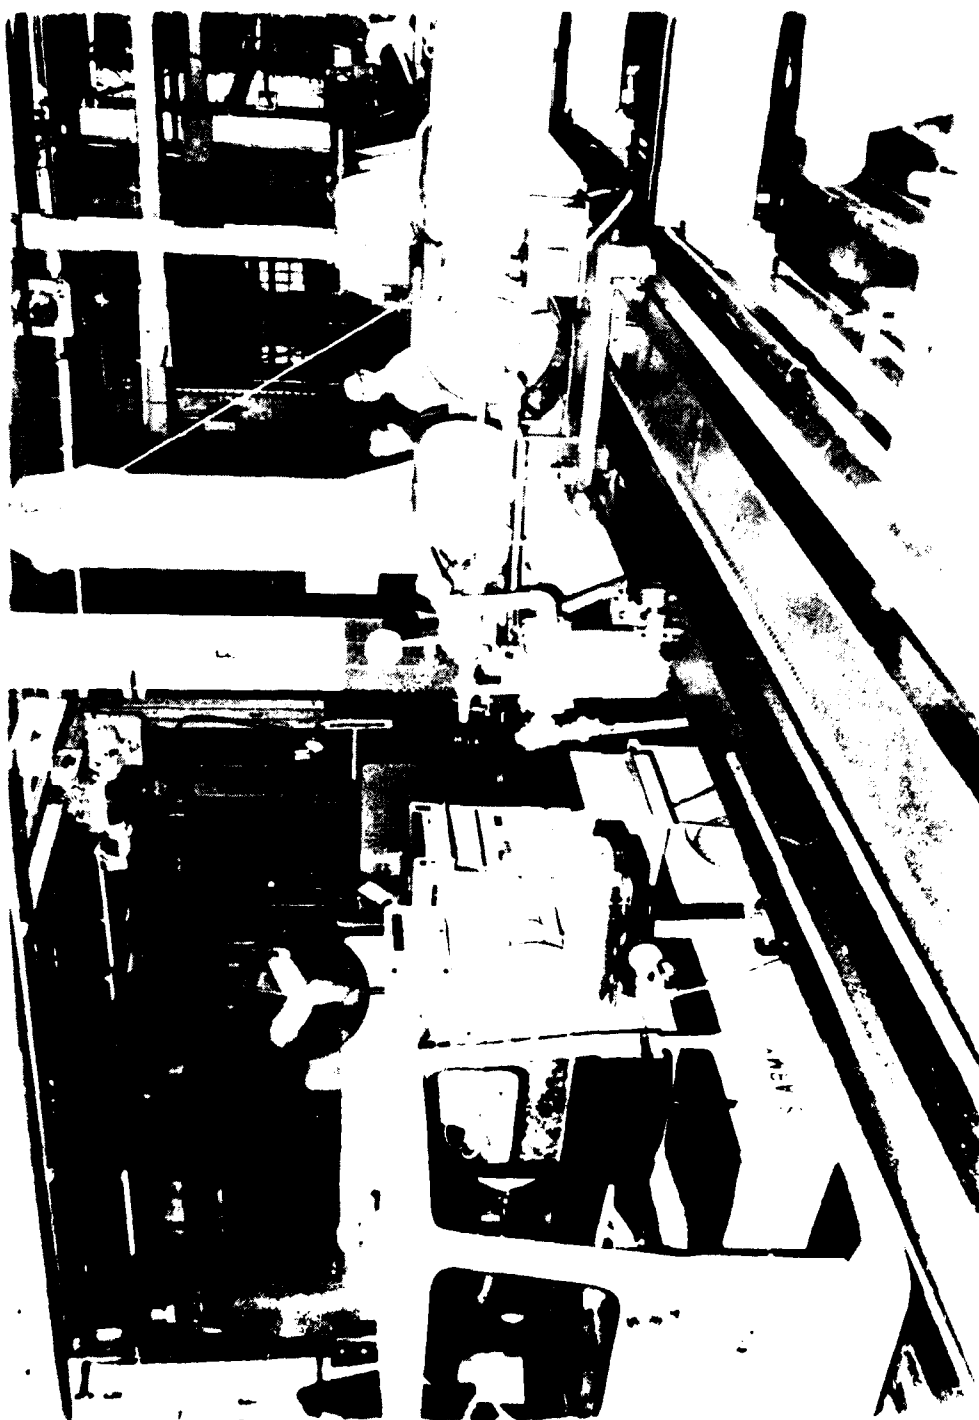


FIGURE 6. CALIBRATION CART
SETUP FOR RIFLING
EAR CALIBRATION

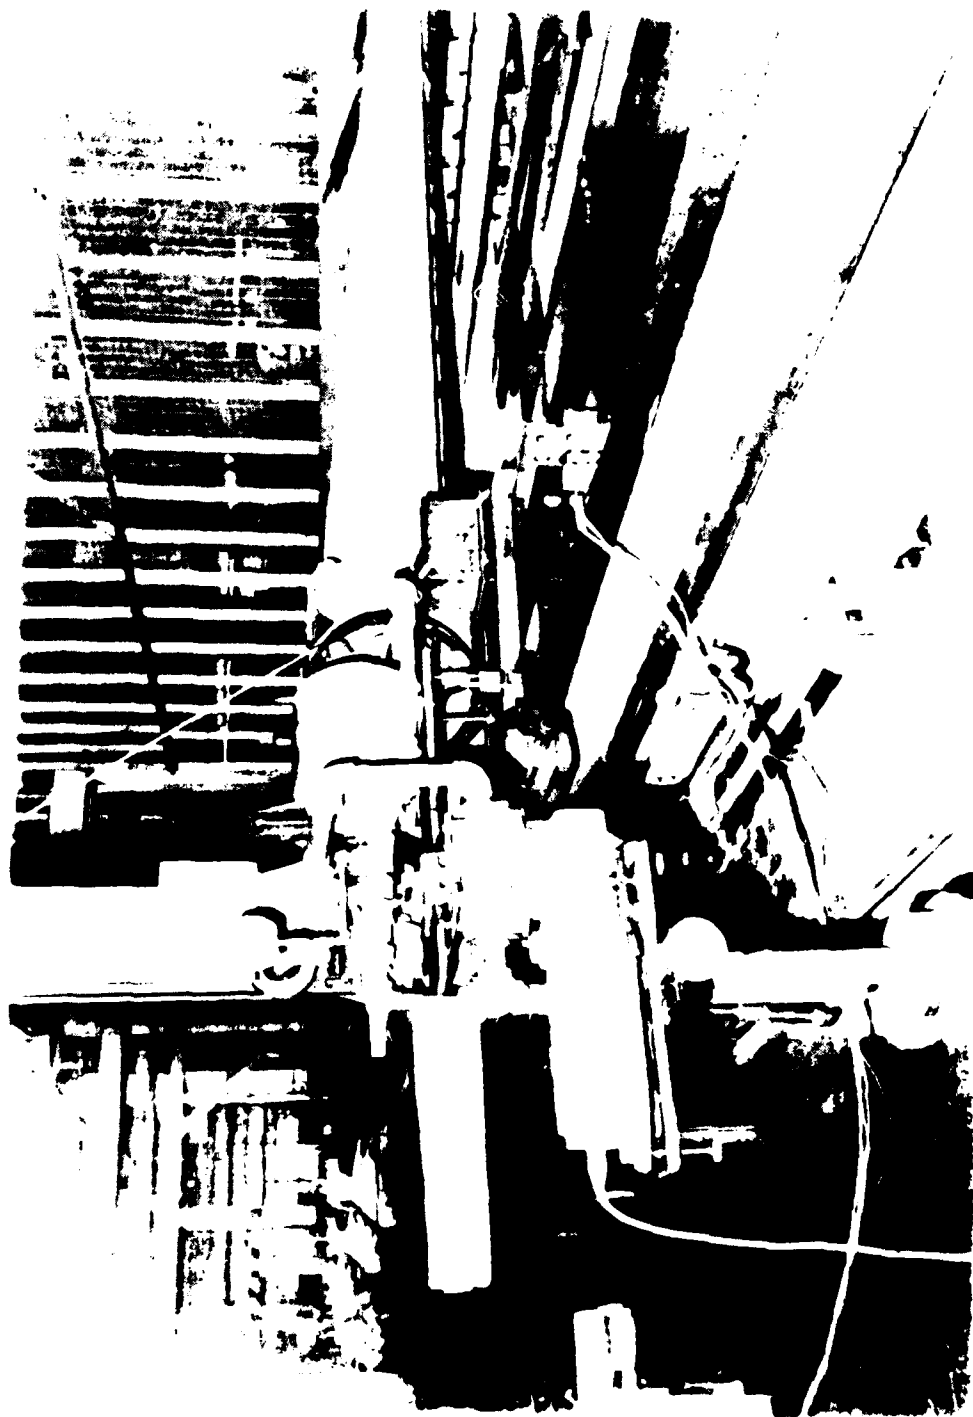


FIGURE 7. LASER HEAD, REMOTE
INTERFEROMETER AND
RETROREFLECTOR

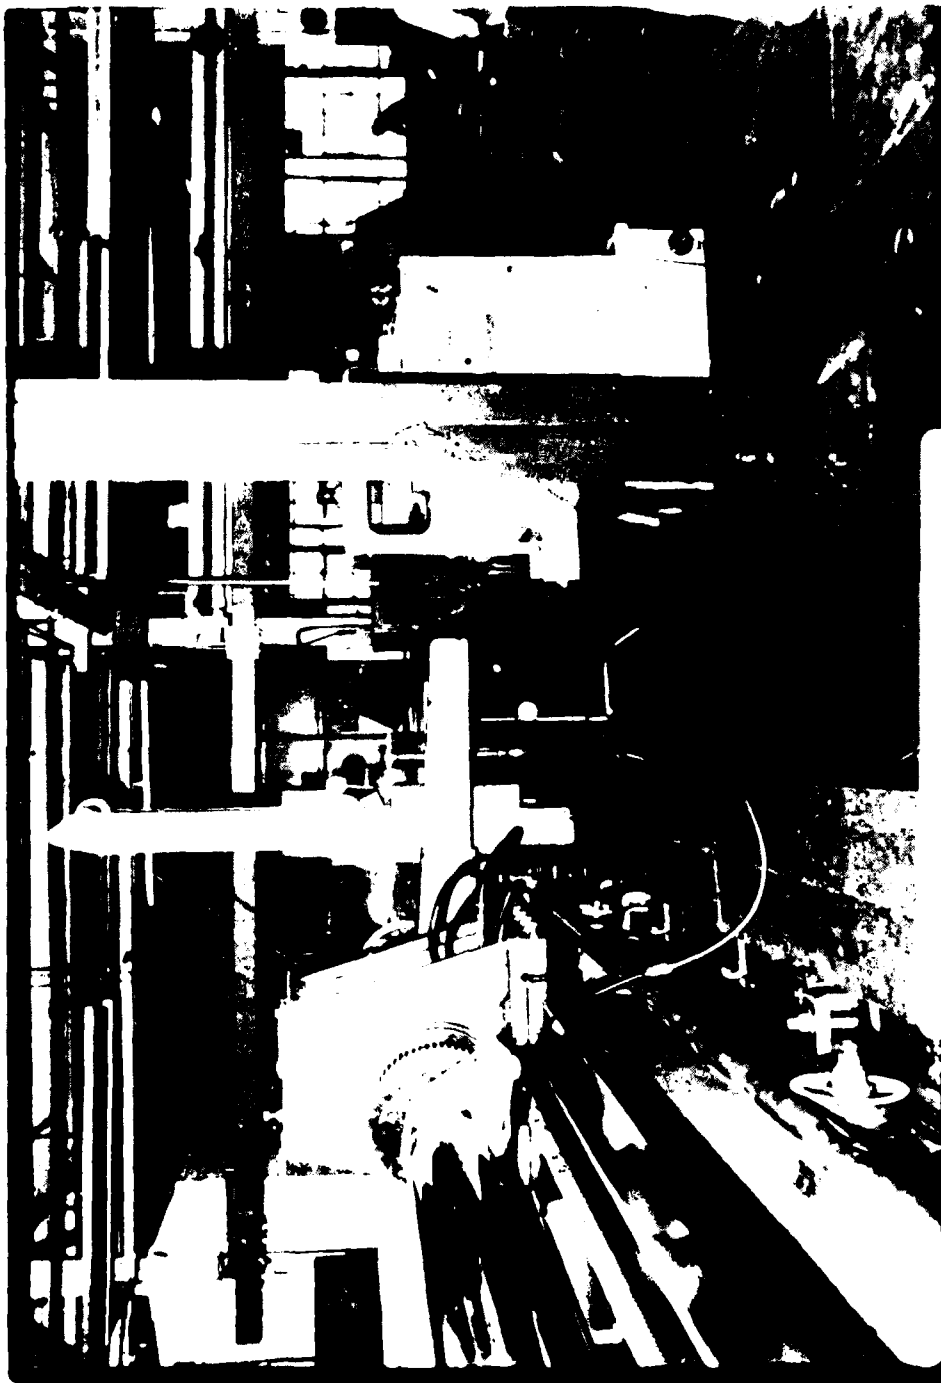


FIGURE 8. RIFLING BAR WITH
ATTACHED ROTARY
ENCODER

To read the rotational movement of the bar, a rotary encoder is strapped to the bar (Fig. 8). A pendulum references the encoder to gravity, and the data from the encoder is fed to the Hewlett Package calculator through the interface, installed on the cart (Fig. 5).

The laser is mounted on a tripod along side the machine bed and aimed at a retroreflector which is sitting on the way of the machine (Figs. 6 & 7). This retroreflector is combined with a beam bender which turns the laser beam 90 degrees and bounces it off the cube corner which sits on the moveable carriage. In this manner, the carriage travel is accurately measured.

The rifling sequence is initiated (the broaches are removed for calibration) and the linear and rotational readings are taken on the fly, automatically, via calculator command. The output is shown in Fig. 9. A program written for the calculator calculates the deviations and prints the inspection report on the spot. Two interpretations are provided; the first converts the deviations to a rotational error in inches at the circumference of the bore for a given downbore distance, the second converts the deviations to a downbore error at a given angular orientation. A second program plots these results, Fig. 10, so that the inspector has a graphic presentation of the inspection results.

This procedure represents a tremendous increase in accuracy and productivity over the previous manual method of calibration using gage blocks and sine bars. In general, the above statement applies wherever an accurate measurement of linear displacements is required. This is especially true if there is no convenient frame of reference available.

RIFLING BAR INSPECTION REPORT

Tube: 105mm M68

Date: 14 Aug. 81

Bar Des. No. *GEAR RIF.*

Bar Insp. No.: *GI-76-1*

Basic Bore Dia. 4.1340

Twist: 1 Turn in 18.0000 Calibers

Down Bore Distance	Total Twist	Non. Circum. Movement	Circum. Error	Down Bore Error
ORIGIN OF RIFLING				
0.0000	0.0000	0.0000	0.0000	0.0000
4.0017	19.3450	0.6284	-0.0005	0.0031
8.0048	38.7700	1.3971	0.0016	-0.0030
11.9951	58.0700	2.0935	0.0014	-0.0030
16.0010	77.3900	2.7927	-0.0008	0.0044
20.0058	96.7350	3.4917	-0.0019	0.0107
23.9988	116.0800	4.1886	-0.0009	0.0050
28.0045	135.4550	4.8877	-0.0010	0.0059
31.9949	154.7250	5.5847	-0.0023	0.0133
35.9984	174.1450	6.2829	-0.0005	0.0027
40.0011	193.5200	6.9815	-0.0001	0.0005
44.0028	212.8700	7.6799	-0.0004	0.0026
48.0042	232.2650	8.3783	0.0009	-0.0050
52.0044	251.5650	9.0765	-0.0010	0.0059
56.0031	270.9050	9.7744	-0.0012	0.0070
59.9945	290.1700	10.4727	-0.0029	0.0164
63.9979	309.5100	11.1709	-0.0039	0.0222
68.0019	328.9650	11.8686	-0.0008	0.0048
71.9942	348.2500	12.5654	-0.0019	0.0109
76.0011	367.6600	13.2647	-0.0010	0.0058
79.9993	386.9750	13.9625	-0.0020	0.0115
83.9978	406.2500	14.6604	-0.0045	0.0259
87.9976	425.6900	15.3585	-0.0013	0.0074
91.9990	444.9750	16.0568	-0.0040	0.0226
96.0005	464.2850	16.7552	-0.0057	0.0328
100.0021	483.7100	17.4537	-0.0034	0.0192
104.0033	502.9150	18.1520	-0.0089	0.0508
108.0035	522.2950	18.8502	-0.0079	0.0451
112.0042	541.5550	19.5484	-0.0113	0.0647
116.0029	561.0400	20.2463	-0.0063	0.0360
120.0043	580.3850	20.9447	-0.0067	0.0387
124.0054	599.7100	21.6430	-0.0079	0.0453
127.9940	619.0400	22.3392	-0.0067	0.0384
131.9979	638.3650	23.0380	-0.0004	0.0479
136.0027	657.7750	23.7370	-0.0071	0.0406
140.0053	677.1350	24.4355	-0.0072	0.0415
143.9976	696.5150	25.1323	-0.0049	0.0280
148.0053	715.9000	25.8318	-0.0050	0.0288
151.9971	735.2300	26.5285	-0.0044	0.0250
155.9979	754.5350	27.2268	-0.0062	0.0355
159.9998	773.8750	27.9252	-0.0070	0.0399
164.0027	793.2300	28.6239	-0.0073	0.0420
167.9935	812.5250	29.3204	-0.0078	0.0446
171.9994	831.9750	30.0196	-0.0053	0.0302
175.9938	851.1700	30.7167	-0.0099	0.0570
179.9984	870.4700	31.4156	-0.0126	0.0722
184.0045	889.9300	32.1148	-0.0098	0.0560
188.0051	909.4550	32.8131	-0.0036	0.0207

FIGURE 9. RIFLING BAR INSPECTION REPORT

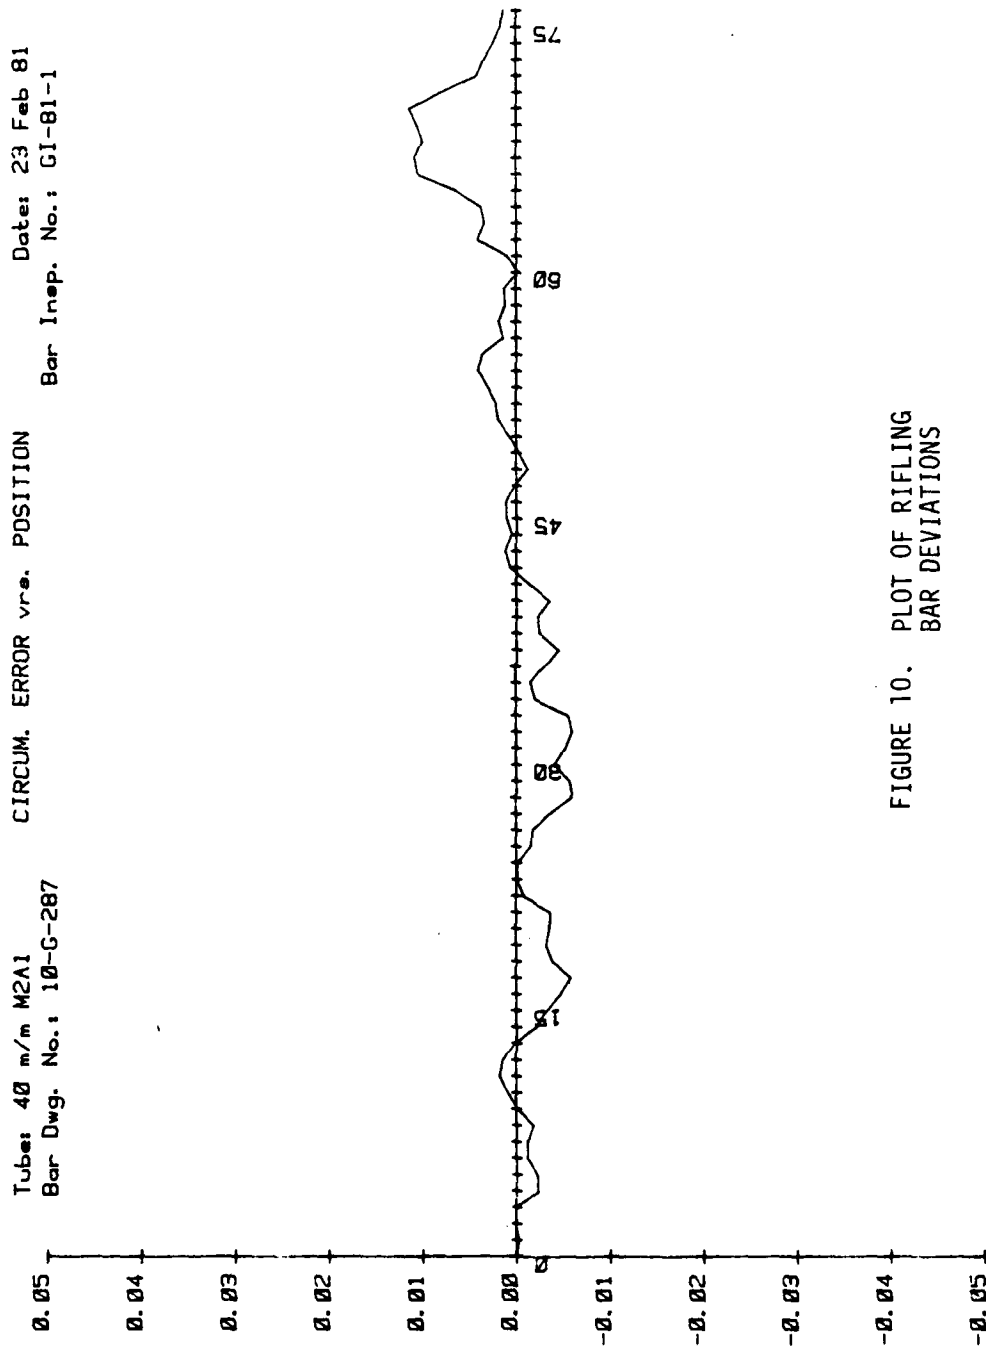


FIGURE 10. PLOT OF RIFLING
BAR DEVIATIONS

5. CONCLUSION

The Remote Laser Interferometer is an extremely versatile tool, which has become an integral part of the calibration system used at the Arsenal. The concept behind the Laser Interferometer Calibration Station would probably have the greatest application in a small precision machine shop where dedicated fixtures could be built for those items requiring frequent calibration, and the precision gained by such a system would justify the cost of a dedicated laser system. Here at Watervliet Arsenal with over 2,000,000 square feet of manufacturing facilities spread over a 140 acre site, such a system has proved unfeasible.

TECHNICAL REPORT INTERNAL DISTRIBUTION LIST

	<u>NO. OF COPIES</u>
COMMANDER	1
TECHNICAL LIBRARY ATTN: DRDAR-LCB-TL	5
DIRECTOR, OPERATIONS DIRECTORATE	2
DIRECTOR, PRODUCT ASSURANCE DIRECTORATE	1
ASSOCIATE DIRECTOR, BENET WEAPONS LABORATORY	2

NOTE: PLEASE NOTIFY COMMANDER, WATERVLIET ARSENAL, ATTN: SARWV-QAE,
WATERVLIET, NY 12189, OF ANY REQUIRED CHANGES.

TECHNICAL REPORT EXTERNAL DISTRIBUTION LIST

	<u>NO. OF COPIES</u>		<u>NO. OF COPIES</u>
ASST SEC OF THE ARMY RESEARCH & DEVELOPMENT ATTN: DEP FOR SCI & TECH THE PENTAGON WASHINGTON, D.C. 20315	1	COMMANDER US ARMY TANK-AUTMV R&D COMD ATTN: TECH LIB-DRDTA-UL WARREN, MICHIGAN 48090	1
COMMANDER US ARMY MAT DEV & READ COMD ATTN: DRCDE 5001 EISENHOWER AVE ALEXANDRIZ, VA 22333	1	COMMANDER US MILITARY ACADEMY ATTN: CHMN, MECH ENGRG DEPT WEST POINT, NY 10996	1
COMMANDER US ARMY ARRADCOM ATTN: DRDAR-LC -TSS (STINFO) DOVER, NJ 07801	1 2	US ARMY MISSILE COMD REDSTONE SCIENTIFIC INFO CEN ATTN: DOCUMENTS SECT, BLG 4484 REDSTONE ARSENAL, AL 35898	2
COMMANDER US ARMY ARRCOM ATTN: DRSAR-QA -IR -LEP-L ROCK ISLAND ARSENAL ROCK ISLAND, IL 61299	1 1 1	COMMANDER US ARMY FGN SCIENCE & TECH CEN ATTN: DRXST-SD 220 7TH STREET, N.E. CHARLOTTESVILLE, VA 22901	1
DIRECTOR US ARMY BALLISTIC RESEARCH LAB ATTN: DRDAR-TSB-S (STINFO) ABERDEEN PROVING GROUND, MD 21005	1	COMMANDER US ARMY MATERIALS & MECHANICS RESEARCH CENTER ATTN: DRXMR-PL -D -FI -S -M -AT WATERTOWN, MA 02172	2 1 1 2 1
COMMANDER US ARMY ELECTRONICS COMD ATTN: TECH LIB FT MONMOUTH, NJ 07703	1		
COMMANDER US ARMY MOBILITY EQUIP R&D COMD ATTN: TECH LIB FT BELVOIR, VA 22060	1		

NOTE: PLEASE NOTIFY COMMANDER, WATERVLIET ARSENAL. ATTN: SARWV-OAE.
WATERVLIET, NY 12189, OF ANY REQUIRED CHANGES.

TECHNICAL REPORT EXTERNAL DISTRIBUTION LIST (CONT.)

	<u>NO. OF COPIES</u>		<u>NO. OF COPIES</u>
COMMANDER US ARMY RESEARCH OFFICE P.O. BOX 12211 RESEARCH TRIANGLE PARK, NC 27709	1	COMMANDER DEFENSE TECHNICAL INFO CENTER ATTN: DTIC-TIR -LTD CAMERON STATION ALEXANDRIA, VA 22314	10 2
COMMANDER US ARMY HARRY DIAMOND LAB ATTN: TECH LIB 2800 POWDER MILL ROAD ADELPHIA, MD 20783			
DIRECTOR US ARMY INDUSTRIAL BASE ENG ACT ATTN: DRXPE-MT ROCK ISLAND, IL	1	DIRECTOR BATTELLE COLUMBUS LAB 505 KING AVE COLUMBUS, OHIO 43201	1
COMMANDER NAVAL SURFACE WEAPONS CEN DAHLGREN, VA 22448	1		
DIRECTOR US NAVAL RESEARCH LAB ATTN: DIR, MECH DIV CODE 26-27 (DOC LIB) WASHINGTON, D.C. 20375	1 1		
NASA SCIENTIFIC & TECH INFO FAC P.O. BOX 8757, ATTN: ACQ BR BALTIMORE/WASHINGTON INTL AIRPORT MARYLAND 21240	1		

NOTE: PLEASE NOTIFY COMMANDER, WATERVLIET ARSENAL, ATTN: SARWV-QAE,
WATERVLIET, NY 12189, OF ANY REQUIRED CHANGES

